



Competitive Selling Guide

An Interactive Tool

NOTE: Products shown may not be available
for importation or sale in every country.



Ankle Fusion

Hammertoe

Jones Fracture


Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation


Ankle Fusion

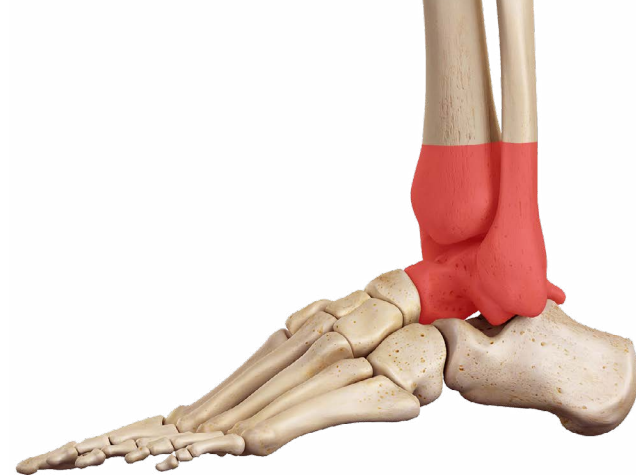

(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Anterior, Lateral and Posterior Approaches	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Smith & Nephew PERI-LOC® Ankle Fusion Plating System</u>
Low profile anterior constructs	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Integra® Tibiaxys® Plating System</u>
Multiple compression options	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Arthrex® Ankle Fusion Plating System</u>
Technique familiarity	<u>DARCO™ Headed Screw System</u>	<u>Synthes Cannulated Screw System – 6.5mm and 7.3mm</u>

Ankle Fusion

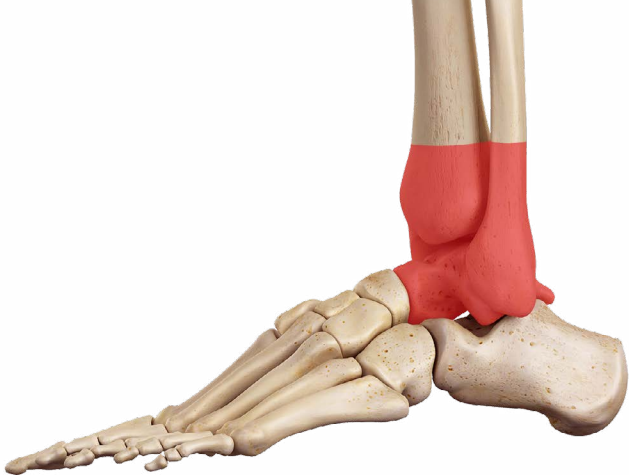

(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Anterior, Lateral and Posterior Approaches	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Smith & Nephew PERI-LOC® Ankle Fusion Plating System</u>
Low profile anterior constructs	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Integra® Tibiaxys® Plating System</u>
Multiple compression options	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Arthrex® Ankle Fusion Plating System</u>
Technique familiarity	<u>DARCO™ Headed Screw System</u>	<u>Synthes Cannulated Screw System – 6.5mm and 7.3mm</u>

ORTHOLOC™ 3Di Ankle Fusion Plating System

Target Surgeon


-
-
-
-

Positioning


-
-
-
-

Exclusive Features

-
-
-

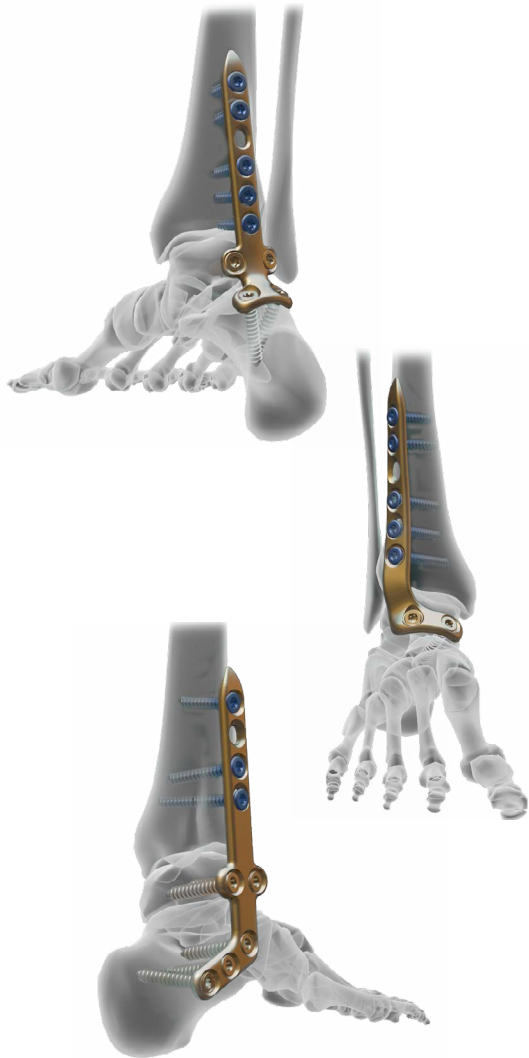

Ankle Fusion

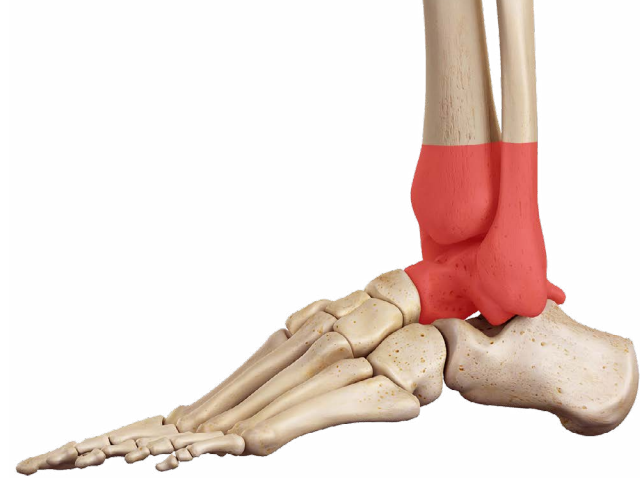

(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Anterior, Lateral and Posterior Approaches	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Smith & Nephew PERI-LOC® Ankle Fusion Plating System</u>
Low profile anterior constructs	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Integra® Tibiaxys® Plating System</u>
Multiple compression options	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Arthrex® Ankle Fusion Plating System</u>
Technique familiarity	<u>DARCO™ Headed Screw System</u>	<u>Synthes Cannulated Screw System – 6.5mm and 7.3mm</u>

DARCO™ Headed Screw System

Target Surgeon

-
-
-
-

Positioning


-

Exclusive Features

-
-



Ankle Fusion

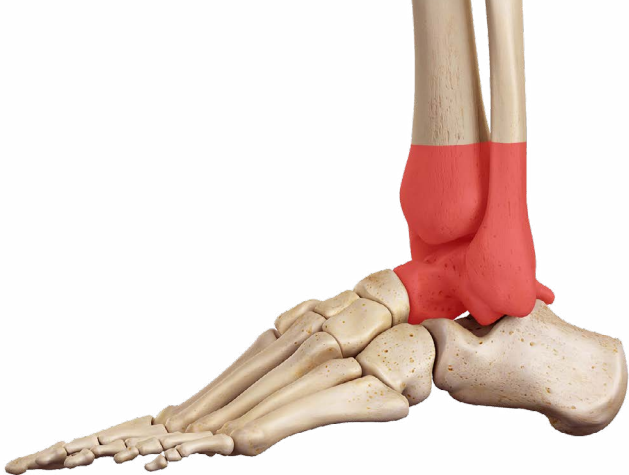

(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Anterior, Lateral and Posterior Approaches	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Smith & Nephew PERI-LOC® Ankle Fusion Plating System</u>
Low profile anterior constructs	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Integra® Tibiaxys® Plating System</u>
Multiple compression options	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Arthrex® Ankle Fusion Plating System</u>
Technique familiarity	<u>DARCO™ Headed Screw System</u>	<u>Synthes Cannulated Screw System – 6.5mm and 7.3mm</u>

Smith & Nephew PERI-LOC® Ankle Fusion Plating System

Target Surgeon

-
-

Positioning

-

Exclusive Features


-
-

Product Information

-
-
-
-



Ankle Fusion

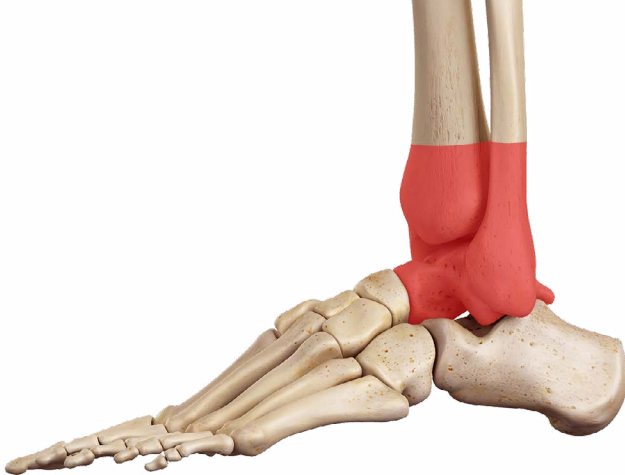

(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Anterior, Lateral and Posterior Approaches	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Smith & Nephew PERI-LOC® Ankle Fusion Plating System</u>
Low profile anterior constructs	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Integra® Tibiaxys® Plating System</u>
Multiple compression options	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Arthrex® Ankle Fusion Plating System</u>
Technique familiarity	<u>DARCO™ Headed Screw System</u>	<u>Synthes Cannulated Screw System – 6.5mm and 7.3mm</u>

Integra® Tibiaxys® Plating System

Target Surgeon

-
-

Positioning

-

Exclusive Features


-
-

Product Information

-
-
-
-



Ankle Fusion

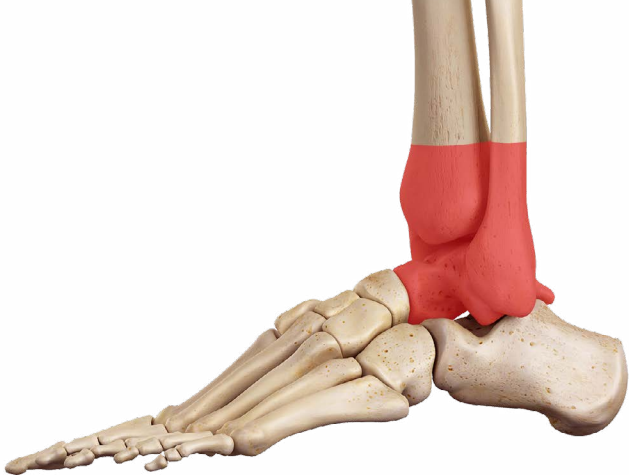

(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Anterior, Lateral and Posterior Approaches	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Smith & Nephew PERI-LOC® Ankle Fusion Plating System</u>
Low profile anterior constructs	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Integra® Tibiaxys® Plating System</u>
Multiple compression options	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Arthrex® Ankle Fusion Plating System</u>
Technique familiarity	<u>DARCO™ Headed Screw System</u>	<u>Synthes Cannulated Screw System – 6.5mm and 7.3mm</u>

Arthrex® Ankle Fusion Plating System

Target Surgeon

-
-

Positioning

-

Exclusive Features


-
-

Product Information

-
-
-
-



Ankle Fusion

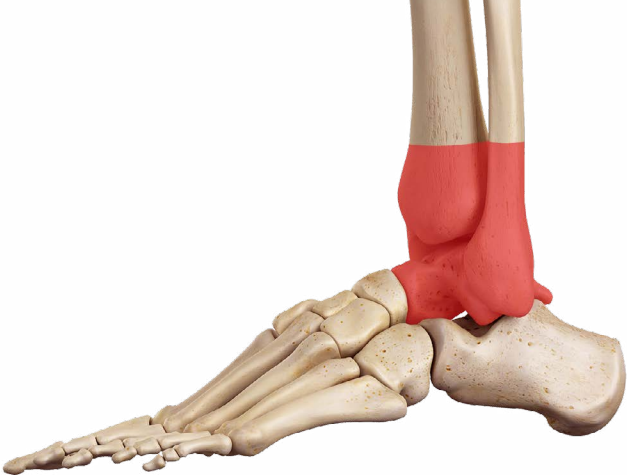

(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Anterior, Lateral and Posterior Approaches	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Smith & Nephew PERI-LOC® Ankle Fusion Plating System</u>
Low profile anterior constructs	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Integra® Tibiaxys® Plating System</u>
Multiple compression options	<u>ORTHOLOC™ 3Di Ankle Fusion</u>	<u>Arthrex® Ankle Fusion Plating System</u>
Technique familiarity	<u>DARCO™ Headed Screw System</u>	<u>Synthes Cannulated Screw System – 6.5mm and 7.3mm</u>

Synthes Cannulated Screw System – 6.5mm and 7.3mm

Target Surgeon

-

Positioning


-

Exclusive Features

-
-

Product Information

-
-
-
-
-
-

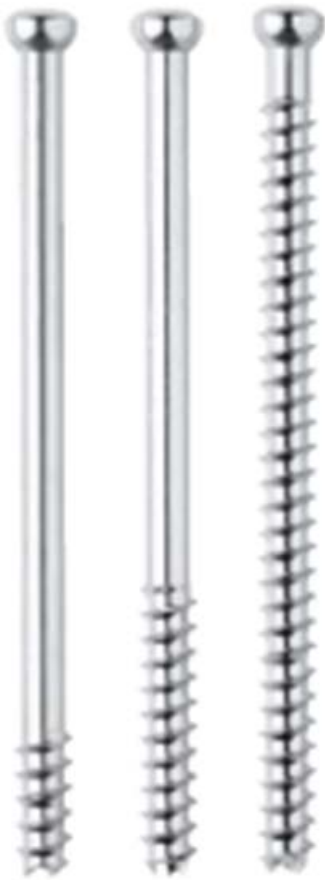

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

PHALINX™

Target Surgeon


-
-
-
-
-

Positioning

-
-

Exclusive Features

-
-
-

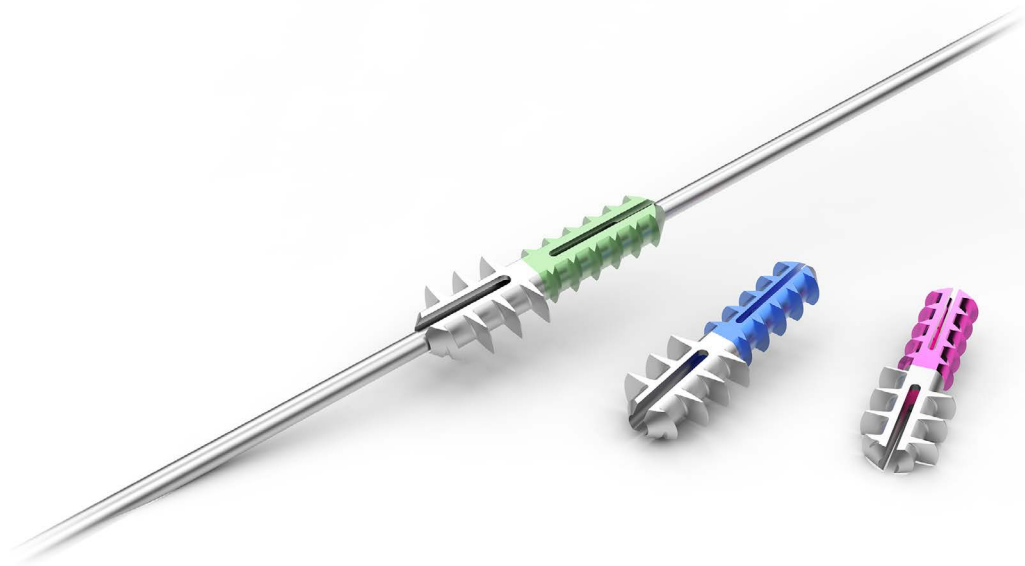

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

PRO-TOE™ VO

Target Surgeon


-
-

Positioning

-

Exclusive Features

-
-

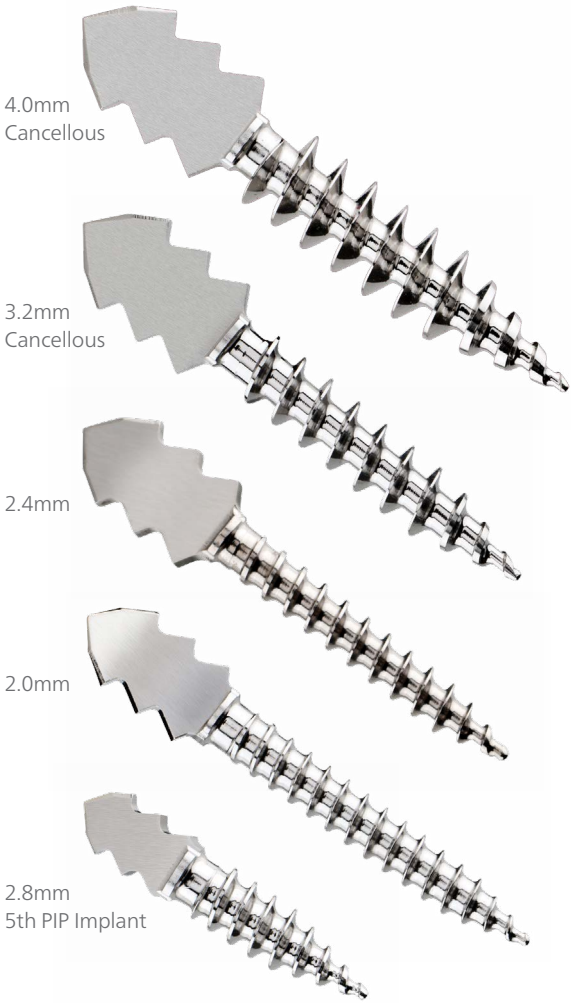

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	PHALINX™	Trilliant® Two-Step OsteoMed® Extremifuse MetaSurg/Integra® DigiFuse®
Low-cost implant	PRO-TOE™ VO	K-wire
Compression	PRO-TOE™ C2	Stryker® Smart Toe® II BME HammerLock® 2
No hardware removal	TENFUSE™ PIP	K-wire Arthrex® Trim-It Spin Pin™

PRO-TOE™ C2

Target Surgeon

-
-

Positioning

-
-

Exclusive Features

-
-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

TENFUSE™ PIP

Target Surgeon


-
-

Positioning

-

Exclusive Features

-
-
-
-

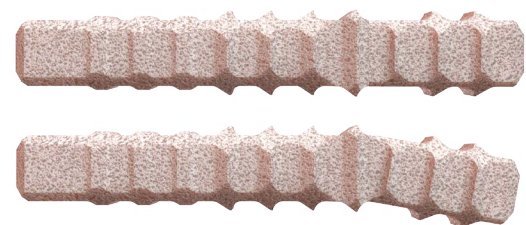

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

Trilliant® Two-Step

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-

Product Information

-
-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

OsteoMed® ExtremiFuse

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-

Product Information

-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	PHALINX™	Trilliant® Two-Step OsteoMed® Extremifuse MetaSurg/Integra® DigiFuse®
Low-cost implant	PRO-TOE™ VO	K-wire
Compression	PRO-TOE™ C2	Stryker® Smart Toe® II BME HammerLock® 2
No hardware removal	TENFUSE™ PIP	K-wire Arthrex® Trim-It Spin Pin™

MetaSurg/Integra® DigiFuse®

Target Surgeon

-
-

Positioning

-
-

Exclusive Features

-

Product Information

-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

K-wire

Target Surgeon

-
-

Positioning

-

Exclusive Features

-

Product Information

-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

Stryker® Smart Toe® II

Target Surgeon

-

Positioning

-

Exclusive Features

-
-
-

Product Information

-
-
-
-



Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

BME HammerLock® 2

Target Surgeon

-

Positioning

-
-

Exclusive Features

-
-
-

Product Information

-
-
-



Hammertoe



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Address MTPJ instability	<u>PHALINX™</u>	<u>Trilliant® Two-Step</u> <u>OsteoMed® Extremifuse</u> <u>MetaSurg/Integra®</u> <u>DigiFuse®</u>
Low-cost implant	<u>PRO-TOE™ VO</u>	<u>K-wire</u>
Compression	<u>PRO-TOE™ C2</u>	<u>Stryker® Smart Toe® II</u> <u>BME HammerLock® 2</u>
No hardware removal	<u>TENFUSE™ PIP</u>	<u>K-wire</u> <u>Arthrex® Trim-It Spin Pin™</u>

Arthrex® Trim-It Spin Pin™

Target Surgeon

-
-

Positioning

-

Exclusive Features


-
-
-

Product Information

-
-



Jones Fracture

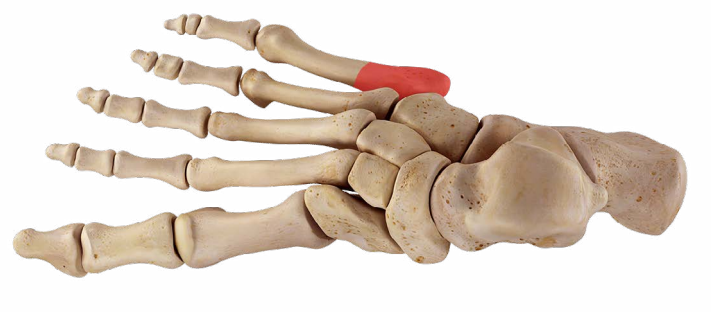

(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Increased implant strength	<u>CHARLOTTE™ CAROLINA™ Jones Fracture Screw System</u>	<u>Arthrex® Jones Fracture System</u>
Low-cost implant	<u>DART-FIRE™ Small Screw System</u>	<u>Stryker® Asnis® III Cannulated Screw System</u>

Jones Fracture



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Increased implant strength	<u>CHARLOTTE™ CAROLINA™ Jones Fracture Screw System</u>	<u>Arthrex® Jones Fracture System</u>
Low-cost implant	<u>DART-FIRE™ Small Screw System</u>	<u>Stryker® Asnis® III Cannulated Screw System</u>

CHARLOTTE™ CAROLINA™ Jones Fracture Screw System

Target Surgeon

-
-
-
-

Positioning

-
-

Exclusive Features

-
-
-



Jones Fracture



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Increased implant strength	<u>CHARLOTTE™ CAROLINA™ Jones Fracture Screw System</u>	<u>Arthrex® Jones Fracture System</u>
Low-cost implant	<u>DART-FIRE™ Small Screw System</u>	<u>Stryker® Asnis® III Cannulated Screw System</u>

Arthrex® Jones Fracture System

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-
-

Product Information

-
-
-
-
-



Jones Fracture



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Increased implant strength	<u>CHARLOTTE™ CAROLINA™ Jones Fracture Screw System</u>	<u>Arthrex® Jones Fracture System</u>
Low-cost implant	<u>DART-FIRE™ Small Screw System</u>	<u>Stryker® Asnis® III Cannulated Screw System</u>

DART-FIRE™ Small Screw System

Target Surgeon

-
-
-
-

Positioning

-
-

Exclusive Features

-
-
-



Jones Fracture



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Increased implant strength	<u>CHARLOTTE™ CAROLINA™ Jones Fracture Screw System</u>	<u>Arthrex® Jones Fracture System</u>
Low-cost implant	<u>DART-FIRE™ Small Screw System</u>	<u>Stryker® Asnis® III Cannulated Screw System</u>

Stryker® Asnis® III Cannulated Screw System

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-

Product Information

-
-
-
-



Midfoot Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Plating System</u>	<u>Depuy-Sythes 2.4mm/2.7mm Variable Angle LCP System</u> <u>Arthrex® CFS System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>
Polyaxial Compression Plating System for simple and complex osteotomies and arthrodesis of the foot	<u>CLAW™ II Polyaxial Compression Plating System</u>	<u>Arthrex® Double Compression Plate System</u>

Midfoot Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Plating System</u>	<u>Depuy-Sythes 2.4mm/2.7mm Variable Angle LCP System</u> <u>Arthrex® CFS System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>
Polyaxial Compression Plating System for simple and complex osteotomies and arthrodesis of the foot	<u>CLAW™ II Polyaxial Compression Plating System</u>	<u>Arthrex® Double Compression Plate System</u>

ORTHOLOC™ 3Di Plating System

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-
-
-



Midfoot Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Plating System</u>	<u>Depuy-Sythes 2.4mm/2.7mm Variable Angle LCP System</u> <u>Arthrex® CFS System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>
Polyaxial Compression Plating System for simple and complex osteotomies and arthrodesis of the foot	<u>CLAW™ II Polyaxial Compression Plating System</u>	<u>Arthrex® Double Compression Plate System</u>

ORTHOLOC™ 3Di CROSSCHECK™ Plating System

Target Surgeon


-
-
-

Positioning

-
-

Exclusive Features

-
-
-

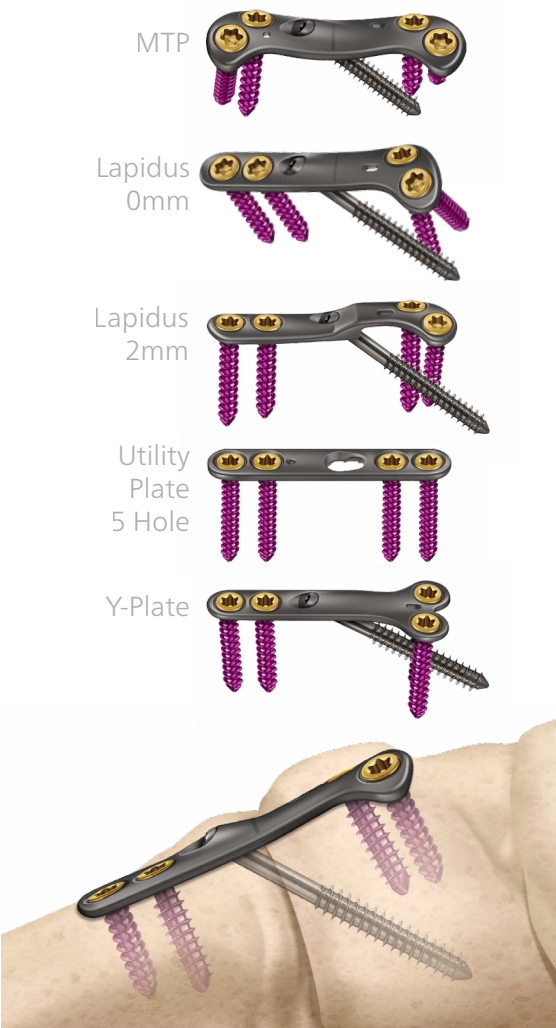

Midfoot Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Plating System</u>	<u>Depuy-Sythes 2.4mm/2.7mm Variable Angle LCP System</u> <u>Arthrex® CFS System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>
Polyaxial Compression Plating System for simple and complex osteotomies and arthrodesis of the foot	<u>CLAW™ II Polyaxial Compression Plating System</u>	<u>Arthrex® Double Compression Plate System</u>

CLAW™ II Polyaxial Compression Plating System

Target Surgeon

-
-

Positioning

-
-

Exclusive Features

-
-
-
-
-
-



Midfoot Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Plating System</u>	<u>Depuy-Sythes 2.4mm/2.7mm Variable Angle LCP System</u> <u>Arthrex® CFS System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>
Polyaxial Compression Plating System for simple and complex osteotomies and arthrodesis of the foot	<u>CLAW™ II Polyaxial Compression Plating System</u>	<u>Arthrex® Double Compression Plate System</u>

Stryker® Anchorage® CP System

Target Surgeon

-

Positioning


-
-

Exclusive Features

-
-
-
-
-

Product Information

-
-
-
-
-

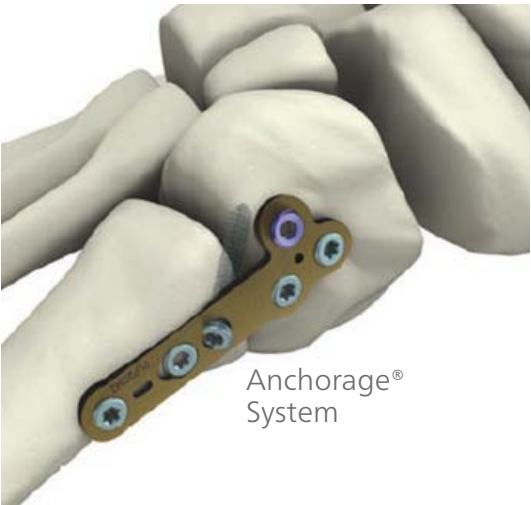

Anchorage® CP System

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Midfoot Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Plating System</u>	<u>Depuy-Sythes 2.4mm/2.7mm Variable Angle LCP System</u> <u>Arthrex® CFS System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>
Polyaxial Compression Plating System for simple and complex osteotomies and arthrodesis of the foot	<u>CLAW™ II Polyaxial Compression Plating System</u>	<u>Arthrex® Double Compression Plate System</u>

Stryker® Anchorage® 2 CP System

Target Surgeon

-

Positioning

-

Exclusive Features

-
-
-
-
-

Product Information

-
-
-
-
-
-

Midfoot Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Plating System</u>	<u>Depuy-Sythes 2.4mm/2.7mm Variable Angle LCP System</u> <u>Arthrex® CFS System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>
Polyaxial Compression Plating System for simple and complex osteotomies and arthrodesis of the foot	<u>CLAW™ II Polyaxial Compression Plating System</u>	<u>Arthrex® Double Compression Plate System</u>

Depuy-Synthes® Variable Angle 2.4/2.7 LCP System

Target Surgeon

-

Positioning

-

Exclusive Features

-
-
-

Product Information

-
-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Midfoot Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Plating System</u>	<u>Depuy-Sythes 2.4mm/2.7mm Variable Angle LCP System</u> <u>Arthrex® CFS System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>
Polyaxial Compression Plating System for simple and complex osteotomies and arthrodesis of the foot	<u>CLAW™ II Polyaxial Compression Plating System</u>	<u>Arthrex® Double Compression Plate System</u>

Arthrex® CFS System

Target Surgeon

-

Positioning

-
-

Exclusive Features

-
-

Product Information

-
-
-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Midfoot Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Plating System</u>	<u>Depuy-Sythes 2.4mm/2.7mm Variable Angle LCP System</u> <u>Arthrex® CFS System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>
Polyaxial Compression Plating System for simple and complex osteotomies and arthrodesis of the foot	<u>CLAW™ II Polyaxial Compression Plating System</u>	<u>Arthrex® Double Compression Plate System</u>

Arthrex® Double Compression Plate System

Target Surgeon

-

Positioning

-
-
-
-

Exclusive Features

-
-

Product Information

-
-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

MTP Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Hallux Plate System</u>	<u>Depuy-Sythes Variable Angle 2.4mm/2.7mm LCP System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>

MTP Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Hallux Plate System</u>	<u>Depuy-Sythes Variable Angle 2.4mm/2.7mm LCP System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>

ORTHOLOC™ 3Di Hallux System

Target Surgeon

-
-
-
-
-
-

Positioning

-
-
-

Exclusive Features

-
-
-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

MTP Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Hallux Plate System</u>	<u>Depuy-Sythes Variable Angle 2.4mm/2.7mm LCP System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>

ORTHOLOC™ 3Di CROSSCHECK™ Plating System

Target Surgeon


-
-
-
-

Positioning

-
-
-
-

Exclusive Features

-
-
-
-
-

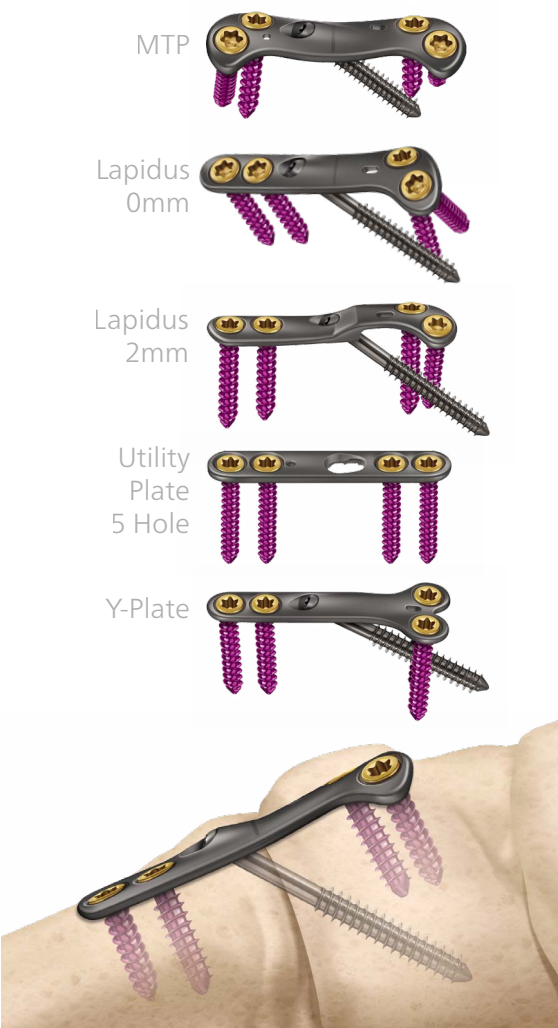

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

MTP Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Hallux Plate System</u>	<u>Depuy-Sythes Variable Angle 2.4mm/2.7mm LCP System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>

Stryker® Anchorage® CP System

Target Surgeon

-

Positioning


-
-

Exclusive Features

-
-
-
-

Product Information

-
-
-
-
-
-
-

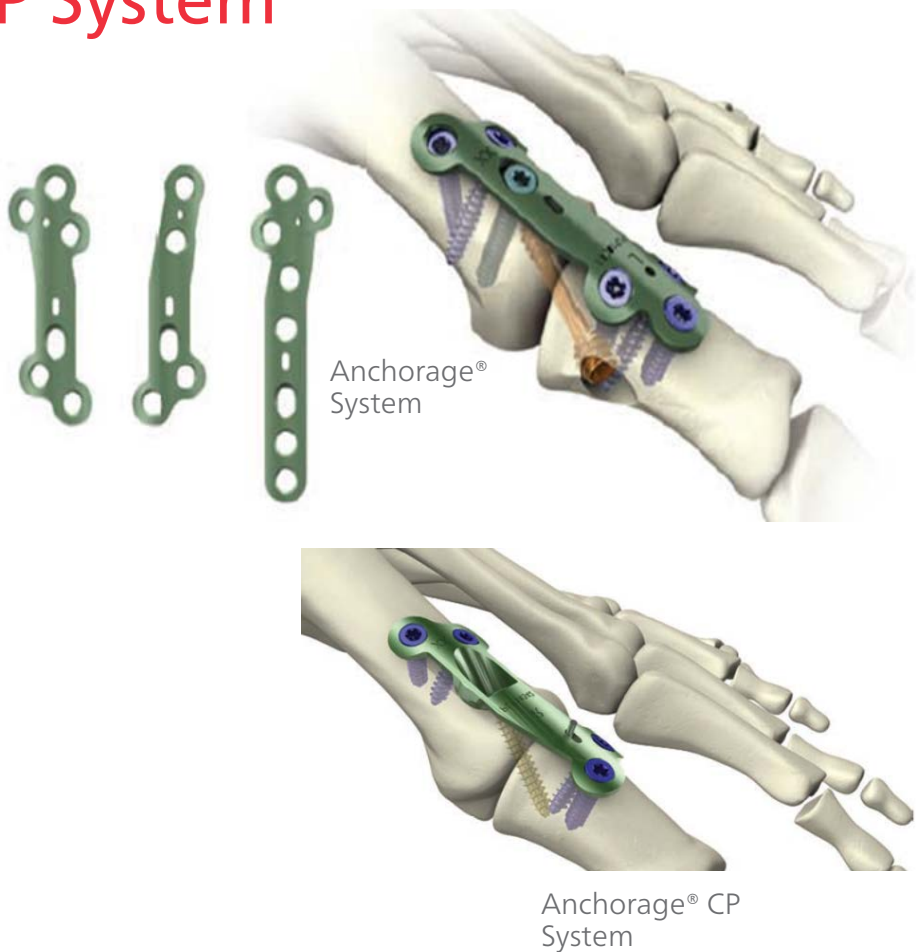

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

MTP Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Hallux Plate System</u>	<u>Depuy-Sythes Variable Angle 2.4mm/2.7mm LCP System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>

Stryker® Anchorage® 2 CP System

Target Surgeon

-

Positioning

-

Exclusive Features

-
-
-
-
-

Product Information

-
-
-
-
-
-

MTP Plating



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Strong, diverse anatomic plating system for the everyday surgeon	<u>ORTHOLOC™ 3Di Hallux Plate System</u>	<u>Depuy-Sythes Variable Angle 2.4mm/2.7mm LCP System</u>
Simple plate with a thin profile featuring Type II Anodization, 3Di Polyaxial Locking Technology and an inter-fragmentary screw through the plate	<u>ORTHOLOC™ 3Di CROSSCHECK™ Plating System</u>	<u>Stryker® Anchorage® CP System</u> <u>Stryker® Anchorage® 2 CP System</u>

Depuy-Synthes® Variable Angle 2.4/2.7 LCP System

Target Surgeon

-

Positioning

-

Exclusive Features

-
-
-
-
-

Product Information

-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

GRAVITY™ Titanium Suture Anchor

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-



*Force Fiber® is a registered trademark of Teleflex® Incorporated

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Insite™ FT (Titanium)

Target Surgeon

-
-

Positioning

-
-

Exclusive Features

-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

G-FORCE™ Tenodesis (PEEK)

Target Surgeon

-
-

Positioning

-
-

Exclusive Features

-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Insite™ FT (PEEK)

Target Surgeon

-
-

Positioning

-
-

Exclusive Features

-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Insite™ FT (Biocomposite)

Target Surgeon

-
-

Positioning

-
-

Exclusive Features

-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Arthrex® FASTak®

Target Surgeon

-

Positioning

-

Exclusive Features

-
-

Product Information

-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Arthrex® Corkscrew®

Target Surgeon

-

Positioning

-

Exclusive Features

-
-
-

Product Information

-
-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Smith & Nephew Twinfix

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-

Product Information

-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Arthrex® Swivelock (PEEK)

Target Surgeon

-

Positioning


-

Exclusive Features

-
-
-

Product Information

-
-
-

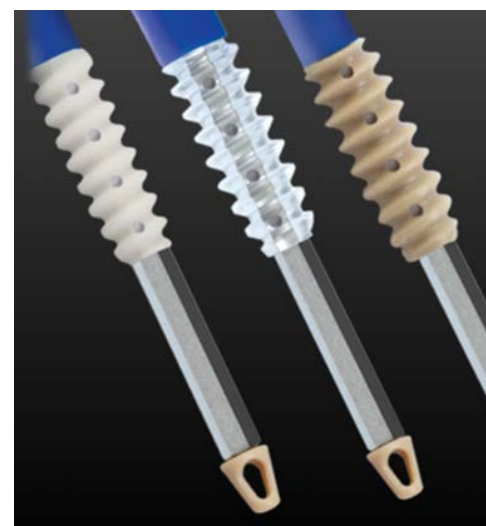

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Smith & Nephew RAPTORMITE™

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-

Product Information

-
-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Soft Tissue



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Metal	<u>GRAVITY™ Titanium Suture Anchor</u> <u>Insite™ FT 2.5/3.5/4.5/5.5</u>	<u>Arthrex® FASTak®</u> <u>Arthrex® Corkscrew®</u> <u>Smith & Nephew Twinfix</u>
PEEK	<u>G-FORCE™ Tenodesis</u> <u>Insite™ FT 4.5/5.5</u> <u>Insite™ FT 4.5/5.5 Knotless</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.0mm</u>
Biocomposite	<u>Insite™ FT 4.5/5.5 (Force Fiber Suture)</u> <u>Insite™ FT 4.5/5/5 (Phantom Fiber™ Suture)</u>	<u>Arthrex® Swivelock</u> <u>Smith & Nephew</u> <u>Twinfix Absorbable</u> <u>Smith & Nephew</u> <u>RAPTORMITE™ 3.7mm</u>

Arthrex® Swivelock (Biocomposite)

Target Surgeon

-

Positioning


-

Exclusive Features

-
-
-

Product Information

-
-
-

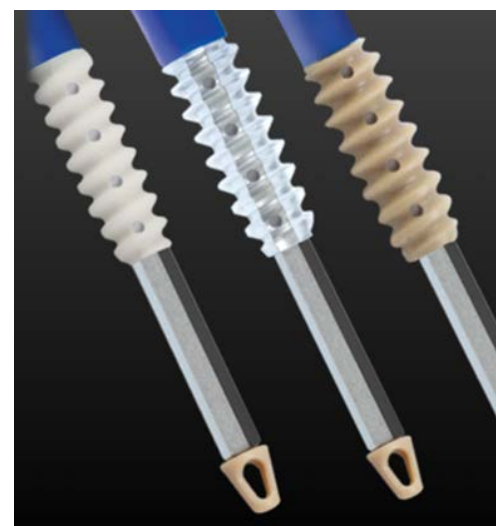

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Staple Fixation



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Low-cost implant	<u>CHARLOTTE™ Quick Staple</u> <u>CHARLOTTE™</u> <u>Compression Staple</u>	<u>BME SPEED™</u>
Compression	<u>CHARLOTTE™</u> <u>Compression Staple</u> <u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>Stryker® EasyClip®</u> <u>BME SPEED™</u>
All-inclusive	<u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>BME SPEED™</u>

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Staple Fixation



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Low-cost implant	<u>CHARLOTTE™ Quick Staple</u> <u>CHARLOTTE™</u> <u>Compression Staple</u>	<u>BME SPEED™</u>
Compression	<u>CHARLOTTE™</u> <u>Compression Staple</u> <u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>Stryker® EasyClip®</u> <u>BME SPEED™</u>
All-inclusive	<u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>BME SPEED™</u>

CHARLOTTE™ Quick Staple

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Staple Fixation



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Low-cost implant	<u>CHARLOTTE™ Quick Staple</u> <u>CHARLOTTE™</u> <u>Compression Staple</u>	<u>BME SPEED™</u>
Compression	<u>CHARLOTTE™</u> <u>Compression Staple</u> <u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>Stryker® EasyClip®</u> <u>BME SPEED™</u>
All-inclusive	<u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>BME SPEED™</u>

CHARLOTTE™ Compression Staple

Target Surgeon

-
-
-

Positioning

-

Exclusive Features

-
-



Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation

Staple Fixation



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Low-cost implant	<u>CHARLOTTE™ Quick Staple</u> <u>CHARLOTTE™</u> <u>Compression Staple</u>	<u>BME SPEED™</u>
Compression	<u>CHARLOTTE™</u> <u>Compression Staple</u> <u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>Stryker® EasyClip®</u> <u>BME SPEED™</u>
All-inclusive	<u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>BME SPEED™</u>

FUSEFORCE™ Nitinol Compression Staple

Target Surgeon

-
-

Positioning

-

Exclusive Features

-
-
-



Staple Fixation



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Low-cost implant	<u>CHARLOTTE™ Quick Staple</u> <u>CHARLOTTE™</u> <u>Compression Staple</u>	<u>BME SPEED™</u>
Compression	<u>CHARLOTTE™</u> <u>Compression Staple</u> <u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>Stryker® EasyClip®</u> <u>BME SPEED™</u>
All-inclusive	<u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>BME SPEED™</u>

Stryker® EasyClip®

Target Surgeon

-

Positioning


-

Exclusive Features

-

Product Information

-
-
-
-

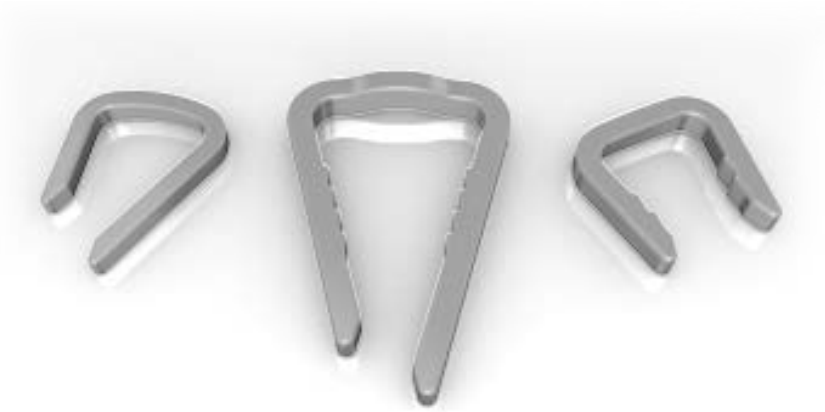

Staple Fixation



(Select product name for further information)

Surgeon Need	Wright Solutions	Competition
Low-cost implant	<u>CHARLOTTE™ Quick Staple</u> <u>CHARLOTTE™</u> <u>Compression Staple</u>	<u>BME SPEED™</u>
Compression	<u>CHARLOTTE™</u> <u>Compression Staple</u> <u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>Stryker® EasyClip®</u> <u>BME SPEED™</u>
All-inclusive	<u>FUSEFORCE™ Nitinol</u> <u>Compression Staple</u>	<u>BME SPEED™</u>

BME SPEED™

Target Surgeon

-
-

Positioning


-

Exclusive Features

-
-

Product Information

-
-



SPEED™



SPEED ARC™



SPEED SHIFT™



SPEED TITAN™



SPEED TRIAD™

Ankle Fusion

Hammertoe

Jones Fracture

Midfoot Plating

MTP Plating

Soft Tissue

Staple Fixation



1023 Cherry Road
Memphis, TN 38117
800 238 7117
901 867 9971
www.wright.com

56 Kingston Road
Staines-upon-Thames
Surrey TW18 4NL
United Kingdom
+44 (0)845 833 4435

161 Rue Lavoisier
38330 Montbonnot Saint Martin
France
+33 (0)4 76 61 35 00

™ and ® denote Trademarks and Registered Trademarks
of Wright Medical Group N.V. or its affiliates.
©2017 Wright Medical Group N.V. or its affiliates.
All Rights Reserved.